
## **Impressions & Construction Bite for Sleep Device**



Maxillary Vestibule should be Captured


The Accu-Dent Syringe works well with Alginate



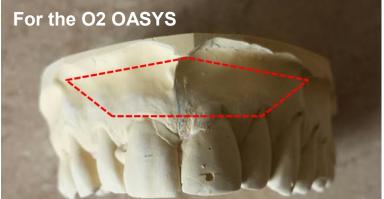

Not Ideal Capture of the Vestibule, but would Trim to Process

Inadequate Clearance and Inadequate Vertical is shown in these Digital Impressions. Advancement and Strength of the Splints are insufficient with the Digital Bite taken.

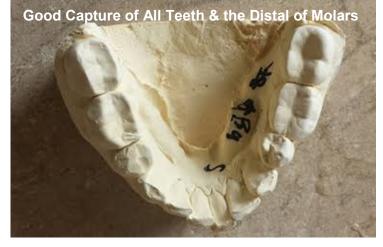



**PVS Impression Capturing the Maxillary Vestibule** 

